



# HT-Air<sup>®</sup> 1200

## Air Supply

---

# User Manual

### TABLE OF CONTENTS

|  |     |
|--|-----|
| Symbol References.....                   | 2   |
| Intended Use and Precautions.....        | 2   |
| Part Identification.....                 | 3   |
| Air Supply Keypad Functions.....         | 3   |
| Product Specifications.....              | 4   |
| Cleaning.....                            | 4   |
| Preventive Maintenance.....              | 4   |
| Infection Control.....                   | 4   |
| Electromagnetic Compatibility Chart..... | 5-7 |
| Returns and Repairs.....                 | 8   |

## Symbol Reference



OPERATING INSTRUCTIONS



THIS END UP



TYPE BF APPLIED PART



TEMPERATURE LIMITATION



ALTERNATING CURRENT



HUMIDITY LIMITATION



MANUFACTURER



DATE OF MANUFACTURE



CAUTION



KEEP DRY



SGS North America Listed Mark

120Vac, 60Hz, 10A

Medical Equipment with respect to electrical shock, fire and mechanical hazards only in accordance with IEC/EN 60601-1.



PROTECTIVE EARTH

---

## Intended Use and Precautions

The HT-Air® 1200 Air Supply provides six airflow options to inflate HoverTech's air-assisted transfer, lift, and positioning devices.

### INTENDED CARE SETTINGS

Hospitals, long-term or extended care facilities

### INTENDED USE


- The caregiver/operator is the person handling the equipment.
- The patient is not the intended operator.

### CAUTIONS

- Route the power cord in a manner to ensure freedom from hazard.
- Avoid blocking the air intakes of the air supply.


- Never leave patient unattended on an inflated device.
- Use this product only for its intended purpose as described in this manual. Only use attachments and/or accessories that are authorized by HoverTech.
- When using the air supply in the MRI environment, a 25-ft. specialty MRI hose is required (available for purchase).
- Avoid electric shock. Do not open air supply.
- Reference product specific user manuals for operating instructions.
- Warning: To avoid the risk of electric shock, this equipment must only be connected to a supply main with protective earth.

## Part Identification

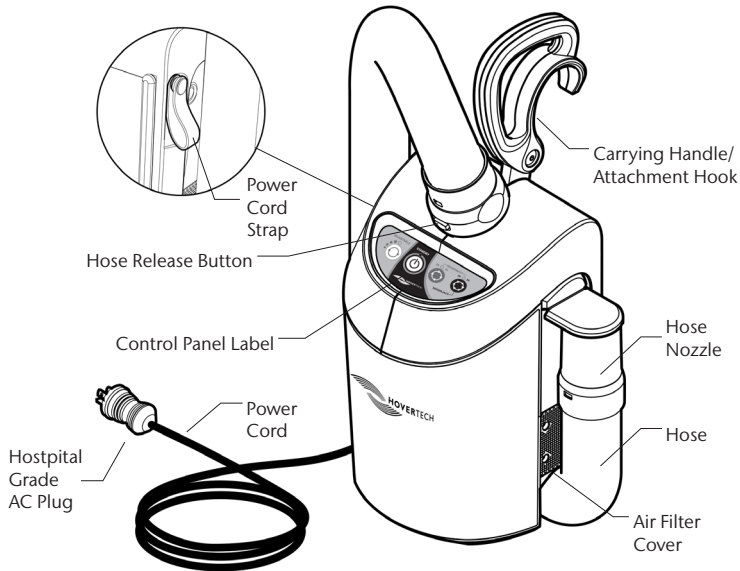

**CAUTION:**  
NO USER SERVICEABLE PARTS.  
Only qualified service personnel shall perform repairs on the HoverTech Air Supply.

## Air Supply Keypad Functions

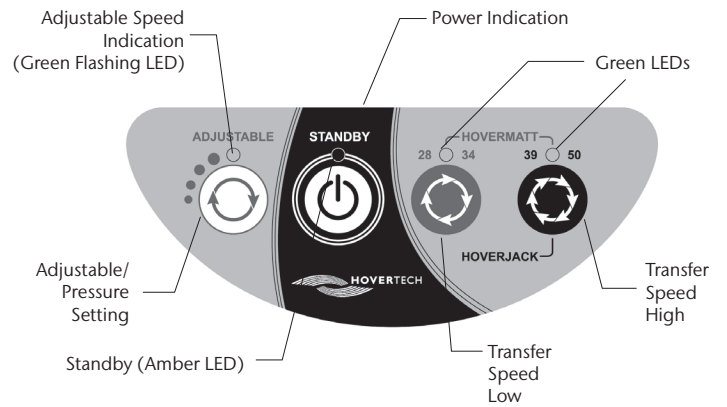

**ADJUSTABLE:** For use with HoverTech air-assisted positioning devices. There are four different settings. Each press of the button increases the air pressure and rate of inflation. The Green Flashing LED will indicate the inflation speed by the number of flashes (i.e. two flashes equals the second inflation speed).

**All of the settings in the ADJUSTABLE range are substantially lower than the HoverMatt and HoverJack settings. The ADJUSTABLE function is not to be used for transferring.**

The ADJUSTABLE setting is a safety feature that can be used to ensure the patient is centered on HoverTech air-assisted devices and to gradually accustom a patient who is timid or in pain to both the sound and functionality of the inflated devices.



**STANDBY:** Used to stop inflation/air flow (Amber LED indicates STANDBY mode).



**HOVERMATT 28/34:** For use with 28" & 34" HoverMatts and HoverSlings.



**HOVERMATT 39/50 & HOVERJACK:** For use with 39" & 50" HoverMatts and HoverSlings and 32" & 39" HoverJacks.

# HT-Air<sup>®</sup> 1200 User Manual

## Product Specifications

|  |  |
|--|--|
| <b>Dimensions:</b>                     | 12.5 x 7 x 7 inches (31.75 x 17.8 x 17.8 cm)       |
| <b>Weight:</b>                         | 12.5 lbs (5.67 kg)                                 |
| <b>Enclosure Material:</b>             | ABS rated UL94V-0/Stainless Steel                  |
| <b>Power Cord Set Length:</b>          | UL Certified<br>15 feet (457 cm)<br>Hospital Grade |
| <b>AC Plug Cord Type &amp; Rating:</b> | SJT 16 AWG*3C, C13 Connector, 15A, 125Vac          |
| <b>Service Life:</b>                   | 5 years  |
| <b>Power Input:</b>                    | 120Vac, 60 Hz, 10 A (North American version)       |

Model #: HTAIR1200 (North American Version) – 120Vac, 60Hz, 10A

**LATEX FREE**

## CLASSIFICATION

Not for use in the presence of flammable anesthetics or in a hyperbaric chamber or oxygen tent.

|  |                           |
|--|---------------------------|
| Type of protection against electric shock:   | CLASS I EQUIPMENT         |
| Degree of protection against electric shock: | TYPE BF APPLIED PART      |
| Protection against ingress of water:         | Ordinary (not protected). |
| Mode of operation:                           | CONTINUOUS OPERATION      |

To remove supply mains, unplug equipment from wall.

## OPERATING CONDITIONS

|                  |                              |
|------------------|------------------------------|
| Use Temperature: | 50° to 104° F (10° to 40° C) |
| Use Humidity:    | 10% to 70% Non-Condensing    |
| Use Altitude:    | 6,562ft / 2,000m             |

|   |                  |
|---|------------------|
| Maximum Operation Atmospheric Pressure Range: | 700 to 1,060 hPa |
|---|------------------|

## STORAGE AND TRANSPORT CONDITIONS

|                               |                                |
|-------------------------------|--------------------------------|
| Storage/Shipping Temperature: | -40° to 158° F (-40° to 70° C) |
| Storage/Shipping Humidity:    | 10% to 70% Non-Condensing      |

## CIRCUIT BREAKER

|                               |                                       |
|-------------------------------|---------------------------------------|
| Max Operating Voltage:        | 32Vdc; 250Vac, 50/60Hz                |
| Current:                      | 12A                                   |
| Operating speed:              | 5 to 30 seconds                       |
| Size:                         | (0.54-0.55) inch x (0.625-0.635) inch |
| Resettable Overload Capacity: | 10x12=120(A)                          |

## Cleaning

Between patient use, clean and disinfect the surface of the air supply by wiping it down with EPA approved hospital-grade disinfectant wipes or disinfectant cleaner sprayed on a cleaning cloth. Follow disinfectant manufacturer's directions for dwell time and other instructions for use. Using the disinfectant wipes/spray cleaner may degrade the graphics on the control panel over time. Replacement panels can be purchased directly from HoverTech, if necessary.

NOTE: DO NOT SPRAY CLEANERS/LIQUIDS DIRECTLY ON THE AIR SUPPLY.

## PREVENTIVE MAINTENANCE

Prior to use, a visual inspection should be performed on the air supply to ensure the power cord is not frayed or nicked and that there is no visual damage that would render the air supply unusable.

If any damage is found that would cause the air supply not to function as intended, the air supply should be removed from use and returned to HoverTech for repair.

The air supply has air filters on either side of the motor. These filters can be accessed by removing the small screws holding the filter covers in place. It is recommended that the air filter is assessed per your facility's preventive maintenance schedule or annually. Filter should be cleaned if clogged. Remove the filter from the air supply and hold it under warm running water. Allow the air filters to dry prior to placing back in the air supply.

The filter should be replaced when it is clogged with debris that does not break free when it is washed. The filter should also be replaced if it begins to lose its shape or deteriorate.



NOTE: IF AIR SUPPLY NEEDS TO BE DISPOSED, CHECK YOUR LOCAL / STATE / FEDERAL / INTERNATIONAL GUIDELINES BEFORE DISPOSAL.

## INFECTION CONTROL

When a HoverTech air supply is used in a patient room where isolation protocols are being observed, the hospital should employ the same protocols/procedures it utilizes for other equipment used in that patient room.

Between use with an airborne isolation patient, the air supply filters can be removed and disinfected or replaced if hospital protocol requires. If the air filters are disinfected, allow them to dry prior to placing back in the air supply.

An air hose cover is available. These covers are disposable and come in a box of 25 (Model #ASHC).

## Electromagnetic Compatibility Chart

### Guidance and manufacturer's declaration – electromagnetic emissions

The HTAIR1200 is intended for use in the electromagnetic environment specified below.

The customer or the user of the HTAIR1200 should assure that it is used in such an environment.

| Emission test  | Compliance | Electromagnetic environment-guidance   |
|--|------------|--|
| RF emissions<br>CISPR 11                                 | Group 1    | The HTAIR1200 uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.   |
| RF emissions<br>CISPR 11                                 | Class A    | The HTAIR1200 is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes. |
| Harmonic emissions<br>IEC 61000-3-2                      | Class A    |  |
| Voltage fluctuations<br>/flicker emissions IEC 61000-3-3 | Compliance |  |

### Guidance and manufacturer's declaration – electromagnetic immunity

The HTAIR1200 is intended for use in the electromagnetic environment specified below.

The customer or the user of the HTAIR1200 should assure that it is used in such an environment.

| Immunity test   | IEC 60601 test level  | Compliance level  | Electromagnetic environment-guidance  |
|---|---|---|---|
| Electrostatic discharge(ESD)<br>IEC 61000-4-2   | ± 6 kV contact<br>± 8 kV air  | ± 6 kV contact<br>± 8 kV air  | Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%            |
| Electrical fast transient/<br>burst IEC 61000-4-4   | ± 2kV for power supply lines<br>± 1kV for input/output lines  | ± 2kV for power supply lines<br>Not applicable  | Mains power quality should be that of a typical commercial or hospital environment.   |
| Surge IEC 61000-4-5   | ± 1kV line(s) to line(s)<br>± 2kV line(s) to earth  | ± 1kV differential mode<br>Not applicable   | Mains power quality should be that of a typical commercial or hospital environment.   |
| Voltage Dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11 | <5% UT(>95% dip in UT) for 0,5 cycle<br>40% UT(60% dip in UT) for 5 cycles<br>70% UT(30% dip in UT) for 25 cycles<br><5% UT(>95% dip in UT) for 5 s | <5% UT(>95% dip in UT) for 0,5 cycle<br>40% UT(60% dip in UT) for 5 cycles<br>70% UT(30% dip in UT) for 25 cycles<br><5% UT(>95% dip in UT) for 5 s | Mains power quality should be that of a typical commercial or hospital environment.   |
| Power frequency (50, 60 Hz) magnetic field IEC 61000-4-8  | 3 A/m   | 3 A/m   | The HTAIR1200 power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment. |


NOTE: UT is the a.c. mains voltage prior to application of the test level.

## Electromagnetic Compatibility Chart

### Guidance and manufacturer's declaration – electromagnetic immunity

The HTAIR1200 is intended for use in the electromagnetic environment specified below.

The customer or the user of the HTAIR1200 should assure that it is used in such an environment.

| Immunity test                 | IEC 60601 test level           | Compliance level | Electromagnetic environment-guidance   |
|-------------------------------|--------------------------------|------------------|--|
| Conducted RF<br>IEC 61000-4-6 | 3 Vrms<br>150 KHz to<br>80 MHz | 3 Vrms           | <p>Portable and mobile RF communications equipment should be used no closer to any part of the HTAIR1200 including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p>Recommended separation distance:</p> $d = 1,2 \sqrt{P}$ $d = 1,2 \sqrt{P} \quad 80\text{MHz to } 800 \text{ MHz}$ $d = 2,3 \sqrt{P} \quad 800\text{MHz to } 2,5 \text{ GHz}$   |
| Radiated RF<br>IEC 61000-4-3  | 3 V/m<br>80MHz to<br>2,5 GHz   | 3 V/m            | <p>Where <math>P</math> is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and <math>d</math> is the recommended separation distance in metres (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, a should be less than the compliance level in each frequency range.<sup>b</sup></p> <p>Interference may occur in the vicinity of equipment marked with the following symbol: </p> |

NOTE1: At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the HTAIR1200 is used exceeds the applicable RF compliance level above, the HTAIR1200 should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the HTAIR1200.

b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

## Electromagnetic Compatibility Chart

### Recommended separation distance between portable and mobile RF communications equipment and the HTAIR1200

The HTAIR1200 is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the HTAIR1200 can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the HTAIR1200 as recommended below, according to the maximum output power of the communications equipment.

| Rated maximum output power of transmitter<br>W | Separation distance according to frequency of transmitter<br>m |  |   |
|--|--|--|---|
|  | 150 kHz to 80 MHz<br>$d = 1,2\sqrt{P}$                         | 80 MHz to 800 MHz<br>$d = 1,2\sqrt{P}$ | 800 MHz to 2,5 GHz<br>$d = 2,3\sqrt{P}$ |
| 0,01   | 0,12   | 0,12                                   | 0,23                                    |
| 0,1  | 0,38   | 0,38                                   | 0,73                                    |
| 1  | 1,2  | 1,2                                    | 2,3                                     |
| 10   | 3,8  | 3,8                                    | 7,3                                     |
| 100  | 12   | 12                                     | 23                                      |

For transmitters rated at a maximum output power not listed above, the recommended separation distance (d) in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where (p) is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE1: At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

## Returns and Repairs

All products being returned to HoverTech must have a Return Goods Authorization (RGA) number issued by the company. Please call 800-471-2776 and ask for a member of the RGA Team, who will issue you an RGA number. Any product returned without an RGA number will cause a delay in the repair time.

Returned products should be sent to:

HoverTech  
Attn: RGA # \_\_\_\_\_  
4482 Innovation Way  
Allentown, PA 18109



4482 Innovation Way  
Allentown, PA 18109

800.471.2776  
Fax 610.694.9601

[HoverTechInternational.com](http://HoverTechInternational.com)  
[Info@HoverTechInternational.com](mailto:Info@HoverTechInternational.com)